


Total bile acids 21 FS

Reliable Assessment of Liver Function

- Excellent recovery of clinically relevant bile acids (target deviation $\leq 7\%$)
- Measuring range up to at least 200 $\mu\text{mol/L}$
- Total confidence in patient results

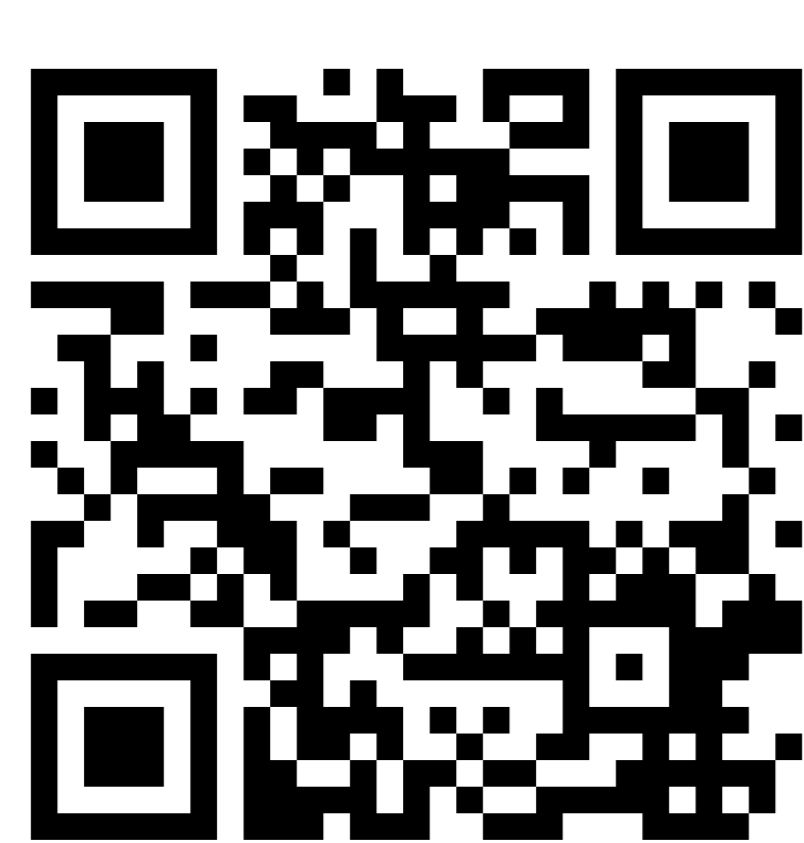

www.diasys-diagnostics.com

